

# Characteristics of the rotor R4-04 for the O4 NCal system VIR-0670A-22

Eddy Dangelser, Dimitri Estevez, Hubert Kocher, Benoit Mours,  
Mehmet Ozturk, Antoine Syx

IPHC-Strasbourg

July 1, 2022

## Contents

<b>1</b>	<b>Introduction</b>	<b>2</b>
<b>2</b>	<b>Measurement method</b>	<b>2</b>
2.1	Thermal effects and density . . . . .	2
<b>3</b>	<b>Raw measurements of the rotor</b>	<b>2</b>
<b>4</b>	<b>Extracting the geometrical parameters</b>	<b>3</b>
4.1	Thickness . . . . .	3
4.2	Radius . . . . .	4
<b>5</b>	<b>Characterization of the rotor using a simple model</b>	<b>5</b>
5.1	Theoretical model of the rotor . . . . .	5
5.2	Thickness . . . . .	5
5.3	Radius . . . . .	6
5.4	Expected NCal signal and uncertainties . . . . .	6
<b>6</b>	<b>Characterization of the rotor using an advanced model</b>	<b>7</b>
6.1	Thickness . . . . .	7
6.2	Radius . . . . .	7
6.3	Counterweight . . . . .	7
6.4	Expected NCal signals and uncertainties . . . . .	8
6.4.1	Advanced geometry including chamfers and counterweight . . . . .	8
6.4.2	Opening angles and sectors asymmetry . . . . .	9
6.4.3	Uncertainties . . . . .	9
<b>A</b>	<b>Appendix</b>	<b>10</b>

## 1 Introduction

This note follows the same discussion made on the rotor R4-01 in [VIR-0591B-22](#). The drawings and figures of the rotor can be found in this technical note.

The rotor has been engraved IPHC-R4-04 on one side and sandblasted on the other side.

## 2 Measurement method

To determine the geometry of the rotor we will use the same method as for R4-01 (see [VIR-0591B-22](#)). The thickness was measured using  $24 \times 2 = 48$  points (see fig. 1), the outer diameter was measured in  $4 \times 2 = 8$  points and the inner diameter using 4 points.

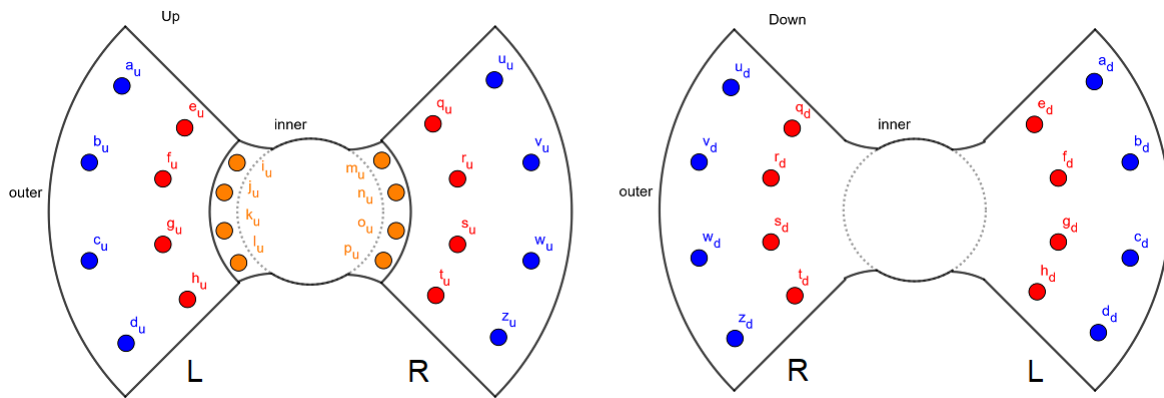


Figure 1: Outline of the faces of the rotor with the measurement points. Left figure is face up, right figure is face down. Sectors have been labelled L for left sector and R for right sector.

The tool used to measure the thickness and the outer diameter is a measuring column "DIGIMAR CX1" (see [VIR-0160A-22](#)) with a given precision of  $2 + L/600 \mu\text{m}$  (L the measured length in mm). A vernier caliper "TESA-CAL IP67" with a precision of  $20 \mu\text{m}$  was used to measure the inner diameter.

The measuring column is operated on the same metrology table than the first rotor. The flatness of the surface was estimated to be  $2.0 \mu\text{m}$  (rms of the measurements).

### 2.1 Thermal effects and density

The rotor R4-04 has been machined from the same aluminum block as R4-01 described in [VIR-0160A-22](#) and was named R4-00 to be a reference cylinder. This cylinder has later been machined to a rotor and is now named R4-04. As for R4-01 the results will be expressed at a reference temperature of  $23^\circ\text{C}$ .

The density of the rotor R4-04 is then  $2808.1 \pm 0.2 \text{ kg}\cdot\text{m}^{-3}$ . This density is measured in air, if the rotor is used under vacuum, the density should be increased by the air density ( $\rho_{air} = 1.3 \text{ kg}\cdot\text{m}^{-3}$ ).

## 3 Raw measurements of the rotor

This section presents the raw measurements made on the rotor at the ambient temperature of  $20.55^\circ\text{C}$ . Table 1 shows the thickness measurements according to the measurement points defined in figure 1. The rotor is

laying on the table. The rotor surface as well as the table are not perfectly flat. Some space could be present in between that should be subtracted when computing the rotor thickness as discussed later.

Measurement point	L sector		Measurement point	R sector	
	Up	Down		Up	Down
a	104.368	104.369	q	104.359	104.347
b	104.357	104.351	r	104.347	104.337
c	104.340	104.337	s	104.339	104.330
d	104.327	104.327	t	104.334	104.327
e	104.360	104.359	u	104.366	104.366
f	104.349	104.342	v	104.343	104.354
g	104.339	104.332	w	104.335	104.343
h	104.336	104.329	z	104.325	104.325
i	101.572		m	101.574	
j	101.571		n	101.571	
k	101.570		o	101.573	
l	101.572		p	101.575	

Table 1: Raw measurements of the height in mm for each point at 20.55°C on L and R sectors of R4-04.

Table 2 displays the diameter measurements. The measurements were made on 4\*2 diameters (two parts of each diameter, the up and down sides of the rotor).

Measurement point	Up	Down
1	208.011	207.988
2	208.017	208.013
3	208.021	208.022
4	208.003	207.981

Table 2: Raw measurements of the diameter in mm for each point at 20.55°C on R4-04.

Measurements were made on the inner radius  $r_{\min} = 28.99$  mm and the up face radius for the counterweight  $r_{\text{counterweight}} = 40$  mm. These values were computed using the vernier caliper and are the same for a temperature of 23°C.

## 4 Extracting the geometrical parameters

### 4.1 Thickness

We need to correct the possible gap between the rotor and the measuring table. Assuming that the table is flatter than the rotor surface we can extract the gap from the measurement of the top surface considering the plane tangents to the highest points (asking them to be on both sectors). For this rotor these points are a, e, u for the up and down faces (see fig. 1). Using the measurements in table 1 we can compute a plane equation for each side of the rotor in cartesian coordinates:

$$\text{Up plane equation : } z = -1.54 \times 10^{-5}x + 4.30 \times 10^{-4}y + 104.35 \quad (1)$$

$$\text{Down plane equation : } z = -1.92 \times 10^{-5}x + 5.30 \times 10^{-4}y + 104.34 \quad (2)$$

Using eqs. (1) and (2) the gap can be determined, see table 3. The maximum rms of the gap of each sector is 15  $\mu\text{m}$ .

Measurement point	L sector		Measurement point	R sector	
	Up	Down		Up	Down
a	0	0	q	0	10
b	-2	1	r	3	9
c	0	3	s	1	5
d	1	10	t	-2	-3
e	0	0	u	0	0
f	3	6	v	9	-5
g	3	5	w	2	-12
h	-3	-3	z	-1	-11

Table 3: Gap computed in  $\mu\text{m}$  on up and down sides of both sectors of R4-04.

We can then compute the rotor thickness for each point by removing these gaps. If one of the raw values is lower than the corrected thickness we take this lowest value. The value of each point is shown in table 4 at 23°C.

Measurement point	L sector	Measurement point	R sector
a	104.281	q	104.312
b	104.292	r	104.318
c	104.306	s	104.328
d	104.325	t	104.342
e	104.295	u	104.307
f	104.306	v	104.322
g	104.306	w	104.337
h	104.321	z	104.353
i	101.578	m	101.580
j	101.577	n	101.577
k	101.576	o	101.579
l	101.578	p	101.581

Table 4: Measurements of the thickness in mm for each point at 23°C on L and R sectors of R4-04.

## 4.2 Radius

Using comparators while the rotor is rotating on its axis we can determine the deformation on both sectors and compute different radii values. Table 5 shows the raw measurements using comparators on L and R sectors. The measurements were made on the up, center and down sides of L and R sectors using three comparators for a total of  $5 \times 3 \times 2 = 30$  points (the first and last points are near the edge of the sectors).

Measurement point	L sector			R sector		
	Up	Center	Down	Up	Center	Down
A	0	0	0	30	10	-10
B	25	20	20	45	25	20
C	35	25	20	40	30	25
D	40	20	15	30	25	20
E	25	5	-50	5	0	5

Table 5: Raw measurements in  $\mu\text{m}$  of the comparators for the L and R sectors of R4-04.

The zeroing of the comparators was made arbitrarily close to the edge of the sector. The offsets shown in table 5 are measured relative to this reference.

To compute the radius per measurement point we use the following process: First we compute the mean deformation for one comparator. Then we remove this mean deformation to each measurement of this comparator. The corrected shift value is added to the mean radius of 104.010 mm computed using table 2 at 23°C. This process is repeated for each comparator. The final radius for each point are shown in table 6.

Measurement point	L sector			R sector		
	Up	Center	Down	Up	Center	Down
A	103.976	103.988	103.997	104.006	103.998	103.987
B	104.001	104.008	104.017	104.021	104.013	104.017
C	104.011	104.013	104.017	104.016	104.018	104.022
D	104.016	104.008	104.012	104.006	104.013	104.017
E	104.001	103.993	103.947	103.981	103.988	104.002

Table 6: Radius measurements in mm at 20.55°C for the L and R sectors of R4-04.

## 5 Characterization of the rotor using a simple model

### 5.1 Theoretical model of the rotor

As explained in VIR-0591B-22 the theoretical strain of the mirror at  $2f$  using FROMAGE v1r2 with the rotor design parameters:

$$\text{strain}(2f) = \frac{2.1198 \times 10^{-18}}{(2f_{rot})^2}$$

This strain value will be compared to models based on the measurements of the rotor.

### 5.2 Thickness

A simple model can be used to determine a mean value for the thickness and its uncertainty.

As shown on fig. 1, a total of 16 points were used to compute the thickness of each sector. In this case we will not consider the inner points so that we obtain uniform sectors.

For the simple model we take the thickness as the mean value of table 4: 104.315 mm at 23°C. Since we have a limited number of measurement points, to be conservative we take the thickness uncertainty as the rms of table 4 (19.5  $\mu\text{m}$ ) to which we add linearly the metrology table uncertainty (2.0  $\mu\text{m}$ ) and the tool uncertainty (2.2  $\mu\text{m}$ ). Therefore, for this simple model, the thickness is  $104.315 \pm 0.024$  mm.

### 5.3 Radius

For the simple model we take the radius as the mean value of table 6: 104.010 mm at 23°C. Using a linear sum of the rms of table 6 (16.4  $\mu\text{m}$ ) and the tool uncertainty (2.4  $\mu\text{m}$ ) we take an uncertainty of 19  $\mu\text{m}$  on the mean radius.

We have to point out that we do not take into account the fact that the sectors might not be centered on the same axis. Therefore the uncertainty might be underestimated. We will then consider each sector individually later.

### 5.4 Expected NCal signal and uncertainties

The geometry used to describe the rotor as a simple model is represented in figure 2.

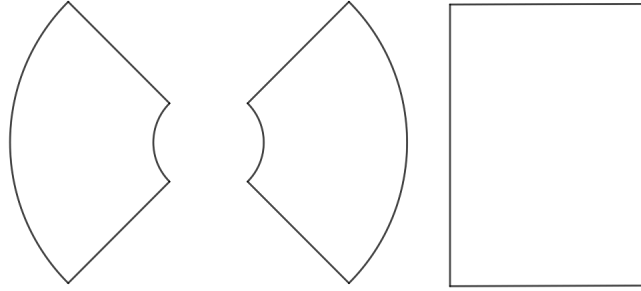


Figure 2: Simple model geometry used to describe the rotor. Left is a front view, right is a side view.

Using the analytical equation of the strain at 2f (see eq.8 in [Newtonian calibrator tests during the Virgo O3 data taking](#)) we compute with our parameters ( $d = 1.7$  m and an angle  $\phi = 34.7^\circ$ ):

$$\text{strain}(2f) = \frac{2.1188 \times 10^{-18}}{(2f_{rot})^2}.$$

Using FROMAGE on this geometry we compute the following 2f strain on the mirror at a distance of 1.7m and an angle of 34.7°:

$$\text{strain}(2f) = \frac{2.1189 \times 10^{-18}}{(2f_{rot})^2}$$

Comparing the theoretical model strain with the simple model at 2f using FROMAGE we obtain a relative deviation of 0.042%.

Comparing the analytical strain at 2f with FROMAGE we obtain a relative deviation of 0.005%.

The uncertainties considered for this model are displayed in table 7.

R4-04 rotor parameter simple model (23°C)			NCal 2f signal uncertainty	
name	value	uncertainty	formula	value (%)
Density $\rho$ (kg.m <sup>-3</sup> )	2808.1	0.2	$\delta\rho/\rho$	0.007
Thickness $b$ (mm)	104.315	$2.4 \times 10^{-2}$	$\delta b/b$	0.023
$r_{max}$ (mm)	104.010	$1.9 \times 10^{-2}$	$4\delta r_{max}/r_{max}$	0.072
$G$ (m <sup>3</sup> .kg <sup>-1</sup> .s <sup>-2</sup> )	$6.67430 \times 10^{-11}$	$1.5 \times 10^{-15}$	$\delta G/G$	0.002
Temperature $T$ (°C)	23	3	$\frac{\partial h}{\partial T} \frac{\Delta T}{h}$	0.014
Total uncertainty from the rotor (quadratic sum)				0.077

Table 7: Uncertainties on the amplitude of the calibration signal at 2f from the R4-04 rotor simple model geometry. The uncertainties from the opening angles are not included.

## 6 Characterization of the rotor using an advanced model

### 6.1 Thickness

A more advanced model can be used considering the deformations on the surfaces of the sectors for better accuracy. Each measurement point of table 4 can be considered as a sub-sector with its own thickness.

The uncertainty on this value is more complex to evaluate. As a conservative approach we use the maximum rms of the deviation to a plane for each sector (6.4  $\mu\text{m}$  see section 4.1) to which we add linearly the uncertainty on the flatness of the measurement table (2.0  $\mu\text{m}$ ) as well as the measurement tool (2.2  $\mu\text{m}$ ). The total uncertainty on the thickness is 11  $\mu\text{m}$ .

### 6.2 Radius

On fig. 1 we divided the external sectors in 4 sub-sectors for each sector (blue points). We convert the point of table 6 to the grid of fig. 1 by averaging the two closest values and converting them to 23°C. The results are shown in table 8. We notice that the R sector is on average 6  $\mu\text{m}$  larger than the L sector.

Radius	L sector			R sector		
	Up	Center	Down	Up	Center	Down
1	103.995	104.004	104.013	104.020	104.011	104.008
2	104.012	104.016	104.023	104.025	104.021	104.026
3	104.020	104.016	104.021	104.017	104.021	104.026
4	104.015	104.006	103.986	104.000	104.006	104.016

Table 8: Radius measurements (in mm at 23°C) for the L and R sectors of R4-04.

The maximum rms of the radii for each sector is 11.2  $\mu\text{m}$ . The tool uncertainty is 2.4  $\mu\text{m}$ . Like for the thickness we use a linear sum and find the uncertainty on both radii to be 14  $\mu\text{m}$ .

### 6.3 Counterweight

A counterweight has been designed to reduce the unbalance of the rotor. This counterweight is made of aluminum 2017 ( $\rho_{\text{Al}_{2017}} = 2790 \text{ kg.m}^{-3}$ ) and the geometry is shown in fig. 3.

The dimensions of the counterweight are: an inner radius of 10 mm, an outer radius of 40 mm and a material cut with a chord of 53.14 mm to balance the rotor (see hatched are on fig. 3).

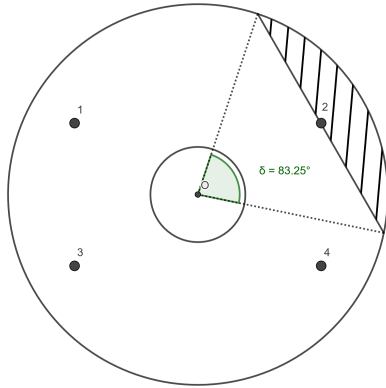


Figure 3: Outline of the counterweight for R4-04. The hatched area represents the material removed.

## 6.4 Expected NCal signals and uncertainties

### 6.4.1 Advanced geometry including chamfers and counterweight

The geometry used to describe the rotor as an advanced model is represented in figure 4. The external parts of the sectors are divided in 3 sub-sectors each to correspond to the different radii determined. In addition we include the counterweight, the screws and screw holes.

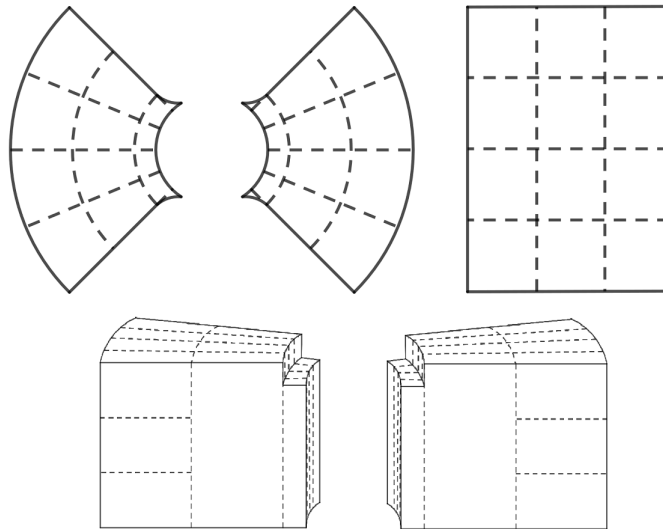


Figure 4: Advanced model geometry used to describe the rotor. Top left is a front view, top right is a side view (external sub-sectors) and bottom is a tilted view of the sectors. Only the 4 external part sectors are divided in 3 sub-sectors each. The chamfers are visible on the inner radius.

Using FROMAGE on this geometry gives the following strains:

- $\text{strain}(1f) = \frac{9.2385 \times 10^{-21}}{(1f_{rot})^2}$
- $\text{strain}(2f) = \frac{2.1182 \times 10^{-18}}{(2f_{rot})^2}$



$$\bullet \text{ strain}(3f) = \frac{2.2940 \times 10^{-23}}{(3f_{rot})^2}$$

The relative deviation to the simple model at 2f is 0.033%.

### 6.4.2 Opening angles and sectors asymmetry

The counterweight is supposed to compensate the unbalance of the rotor at 1f. As the 1f signal from section 6.4.1 is a bit more than a factor 8 smaller than R4-01 we will consider an error of  $0.047\%/8=0.006\%$  on the 2f signal for R4-04 due to the opening angle and asymmetry.

### 6.4.3 Uncertainties

Comparing the advanced model of the rotor + chamfers + screw holes ( $\text{strain}(2f) = 2.1183 \times 10^{-18}/(2f_{rot})^2$ ) to the simple model gives a relative deviation of 0.028%. This deviation will be considered as our modelling uncertainty.

The uncertainties considered for this full model are displayed in table 9.

R4-04 rotor parameter advanced model (23°C)			NCal 2f signal uncertainty	
name	mean value	uncertainty	formula	value (%)
Density $\rho$ (kg.m <sup>-3</sup> )	2808.1	0.2	$\delta\rho/\rho$	0.007
Thickness $b$ left sector (12 sub-sectors) (mm)	104.303	$1.1 \times 10^{-2}$	$\delta b/b$	0.010
Thickness $b$ right sector (12 sub-sectors) (mm)	104.327			
$r_{max}$ left sector (12 ext sub-sectors) (mm)	104.010	$1.4 \times 10^{-2}$	$4\delta r_{max}/r_{max}$	0.052
$r_{max}$ right sector (12 ext sub-sectors) (mm)	104.016			
$G$ (m <sup>3</sup> .kg <sup>-1</sup> .s <sup>-2</sup> )	$6.67430 \times 10^{-11}$	$1.5 \times 10^{-15}$	$\delta G/G$	0.002
Temperature $T$ (°C)	23	3	$\left  \frac{\partial h}{\partial T} \right  \frac{\Delta T}{h}$	0.014
Modelling Uncertainty				0.028
Opening angle and asymmetry uncertainty				0.006
Total uncertainty from the rotor (quadratic sum)				0.062

Table 9: Uncertainties on the amplitude of the calibration signal at 2f from the R4-04 rotor advanced model geometry at 23°C.

**A Appendix**

```
### This is a cfg file for a more realistic geometry of the mirror and the Virgo NCal for O4 (2022)
```

```
### ALL THE OBJECTS ARE DEFINED IN THE MIRROR'S FRAME (0,x,y,z),
### with 0 the center of the mirror, x axis along the ITF's beam toward the beam-splitter,
### y axis orthogonal to x in the plane of the ITF,
### z axis orthogonal to the plane of the ITF upward
```

```
### MIRROR DEFINITION
```

```
GRID_SIZE 12 30 8
```

```
CYLINDER 2202. 0 0.175 0.2 360 0 0 0
```

```
GRID_SIZE 1 1 1
```

```
# Defining the flats on the edge of the mirror
```

```
CUT_CYL 2202. 0.175 0.2 0.05 0 0
```

```
CUT_CYL 2202. 0.175 0.2 0.05 0 180
```

```
# Defining the ears and anchors of the mirror
```

```
CUBOID 2202. 0.090 0.010 0.015 0 0.1782 -0.0125
```

```
CUBOID 2202. 0.090 0.010 0.015 0 -0.1782 -0.0125
```

```
CUBOID 2202. 0.039 0.008 0.008 -0.02 -0.1772 -0.024
```

```
CUBOID 2202. 0.039 0.008 0.008 -0.02 0.1772 -0.024
```

```
CUBOID 2202. 0.039 0.008 0.008 0.02 -0.1772 -0.024
```

```
CUBOID 2202. 0.039 0.008 0.008 0.02 0.1772 -0.024
```

```
### ROTOR DEFINITION: CYLINDER DENSITY INNER_RADIUS OUTER_RADIUS THICKNESS OPEN_ANGLE r z theta
```

```
ROTOR_CYLINDRICAL 1.7 34.7 0 0
```

```
### COUNTERWEIGHT 2790.
```

```
GRID_SIZE 16 65 40
```

```
CYLINDER 2790. 0.010 0.040 0.003 360 0 0.049546 0
```

```
GRID_SIZE 1 1 1
```

```
CUT_CYL 2790. 0.040 0.002 0.05314 0 30
```

```
### SCREW HOLES
```

```
GRID_SIZE 4 4 4
```

```
CYLINDER -2808.1 0 0.0015 0.012 360 0.03 0.04478893644652 150
```

```
CYLINDER -2808.1 0 0.0015 0.012 360 0.03 0.04478893644652 30
```

```
CYLINDER -2808.1 0 0.0015 0.012 360 0.03 0.04478993650434 210
```

```
CYLINDER -2808.1 0 0.0015 0.012 360 0.03 0.04479043653325 330
```

```
### SCREWS COUNTERWEIGHT
```

```
CYLINDER 4810. 0 0.0015 0.003 360 0.03 0.0495463318739 150
```

```
CYLINDER 7600. 0 0.0015 0.00665 360 0.03 0.04746543653325 150
```

```
CYLINDER 4810. 0 0.0015 0.003 360 0.03 0.0495463318739 30
```

```
CYLINDER 7600. 0 0.0015 0.00665 360 0.03 0.04746543653325 30
```

```
CYLINDER 4810. 0 0.0015 0.003 360 0.03 0.0495463318739 210
```

```
CYLINDER 7600. 0 0.0015 0.00665 360 0.03 0.04746543653325 210
```

```
CYLINDER 4810. 0 0.0015 0.003 360 0.03 0.0495463318739 330
CYLINDER 7600. 0 0.0015 0.00665 360 0.03 0.04746543653325 330

# TRES RAPIDE
#GRID_SIZE 4 4 4
# RAPIDE
#GRID_SIZE 8 17 14
# LENT
GRID_SIZE 8 65 40

### L sector

## Inner part
OUTER_FILLET 2808.1 0.02899 0.101578 -0.002726 0.01 -11.25 146.25
CYLINDER 2808.1 0.02899 0.04 0.101578 22.5 0 -0.002726 146.25
CYLINDER 2808.1 0.02899 0.04 0.101577 22.5 0 -0.002727 168.75
CYLINDER 2808.1 0.02899 0.04 0.101576 22.5 0 -0.002726 191.25
CYLINDER 2808.1 0.02899 0.04 0.101578 22.5 0 -0.002726 213.75
OUTER_FILLET 2808.1 0.02899 0.101578 -0.002726 0.01 11.25 213.75

## Middle part
CYLINDER 2808.1 0.04 0.072003 0.104295 22.5 0 0 146.25
CYLINDER 2808.1 0.04 0.072003 0.104295 22.5 0 0 168.75
CYLINDER 2808.1 0.04 0.072003 0.104306 22.5 0 0 191.25
CYLINDER 2808.1 0.04 0.072003 0.104321 22.5 0 0 213.75

## Outer part
CYLINDER 2808.1 0.072003 0.103995 0.0347603430601667 22.5 0 0.0347603430601667 146.25
CYLINDER 2808.1 0.072003 0.104004 0.0347603430601667 22.5 0 0 146.25
CYLINDER 2808.1 0.072003 0.104013 0.0347603430601667 22.5 0 -0.0347603430601667 146.25

CYLINDER 2808.1 0.072003 0.104012 0.03476400993884 22.5 0 0.03476400993884 168.75
CYLINDER 2808.1 0.072003 0.104016 0.03476400993884 22.5 0 0 168.75
CYLINDER 2808.1 0.072003 0.104023 0.03476400993884 22.5 0 -0.03476400993884 168.75

CYLINDER 2808.1 0.072003 0.104020 0.0347686768753333 22.5 0 0.0347686768753333 191.25
CYLINDER 2808.1 0.072003 0.104016 0.0347686768753333 22.5 0 0 191.25
CYLINDER 2808.1 0.072003 0.104021 0.0347686768753333 22.5 0 -0.0347686768753333 191.25

CYLINDER 2808.1 0.072003 0.104015 0.03477501057486 22.5 0 0.03477501057486 213.75
CYLINDER 2808.1 0.072003 0.104006 0.03477501057486 22.5 0 0 213.75
CYLINDER 2808.1 0.072003 0.103986 0.03477501057486 22.5 0 -0.03477501057486 213.75

### R sector

## Inner part
OUTER_FILLET 2808.1 0.02899 0.101580 -0.002745 0.01 11.25 33.75
CYLINDER 2808.1 0.02899 0.04 0.101580 22.5 0 -0.002745 33.75
CYLINDER 2808.1 0.02899 0.04 0.101577 22.5 0 -0.002748 11.25
CYLINDER 2808.1 0.02899 0.04 0.101579 22.5 0 -0.002746 348.75
CYLINDER 2808.1 0.02899 0.04 0.101581 22.5 0 -0.002744 326.25
OUTER_FILLET 2808.1 0.02899 0.101581 -0.002744 0.01 -11.25 326.25

## Middle part
CYLINDER 2808.1 0.04 0.072003 0.104312 22.5 0 0 33.75
CYLINDER 2808.1 0.04 0.072003 0.104318 22.5 0 0 11.25
```

CYLINDER 2808.1 0.04 0.072003 0.104328 22.5 0 0 348.75  
CYLINDER 2808.1 0.04 0.072003 0.104342 22.5 0 0 326.25

## ## Outer part

CYLINDER 2808.1 0.072003 0.104020 0.03476901022794 22.5 0 0.03476901022794 33.75  
CYLINDER 2808.1 0.072003 0.104011 0.03476901022794 22.5 0 0 33.75  
CYLINDER 2808.1 0.072003 0.104008 0.03476901022794 22.5 0 -0.03476901022794 33.75

CYLINDER 2808.1 0.072003 0.104025 0.03477401051704 22.5 0 0.03477401051704 11.25  
CYLINDER 2808.1 0.072003 0.104021 0.03477401051704 22.5 0 0 11.25  
CYLINDER 2808.1 0.072003 0.104026 0.03477401051704 22.5 0 -0.03477401051704 11.25

CYLINDER 2808.1 0.072003 0.104017 0.03477901080614 22.5 0 0.03477901080614 348.75  
CYLINDER 2808.1 0.072003 0.104021 0.03477901080614 22.5 0 0 348.75  
CYLINDER 2808.1 0.072003 0.104026 0.03477901080614 22.5 0 -0.03477901080614 348.75

CYLINDER 2808.1 0.072003 0.104000 0.0347842555092455 22.5 0 0.0347842555092455 326.25  
CYLINDER 2808.1 0.072003 0.104006 0.0347842555092455 22.5 0 0 326.25  
CYLINDER 2808.1 0.072003 0.104016 0.0347842555092455 22.5 0 -0.0347842555092455 326.25

## ### GENERAL PARAMETERS

STEP 22.5 16

ARM\_LENGTH 3000

SIGNAL 3